DP2 SERIES

High-performance Digital Pressure Sensor









Complete functionality! Selection from a wide **lineup**

Passed the UL 991 Environment Test





UL 61010C-1 compatible, Passed the UL 991 Environment Test based on SEMI S2-0200. [Category applicable for semiconductor manufacturing: TWW2, Process Equipment] [Applicable standards: UL 61010C-1] [Additional test / evaluation standards as per intended use: UL991, SEMI S2-0200]

High accuracy • high resolution • high speed

It achieves a 2.5 ms, or less, response time at a high resolution of 1/1,000. It enables highly accurate sensing with its excellent repeatability and temperature characteristics.

Response time





Clearly visible LED display with 31/2 digits

Bright red LED 7-segment display having 31/2 digits, 10 mm 0.394 in high. The displayed figures are remarkably noticeable not only in a dark area, but also in a well-lit place.




Setting with easy key operation

Initialization and threshold value settings are easily done by key operation while seeing the values on the display.




Four output modes enable versatile pressure level control

1 Hysteresis mode




The common hysteresis of the comparative outputs can be set, as desired, with the set values.

3 Dual output mode




The outputs can be put to different use, such as, detection of different kinds of objects, control function, alarm function etc.

2 Window comparator mode



The comparative outputs can be turned ON or OFF by a pressure which is within the pressure range set by Set Value 1 and Set Value 2.

4 Automatic sensitivity setting mode




Using actual objects, if the pressure values for OK objects and NG objects are input, then the sensor is automatically set to the optimum pressure value (mid-value).

Selection from six pressure units

The pressure unit can be selected from six different systems to suit your requirement.

The selectable pressure units differ with the sensor type. When the pressure unit is changed, the measured pressure value and the set values are automatically converted.




Note: 'MPa' in case of DP2-22□, DP2-42□ and DP2-62□.

APPLICATIONS


Confirmation of chip component suction

The light weight type does not disturb the movement of the suction head, even if it is mounted close to the head.




Verifying placement of frame

High pressure is attained when the frame is exactly seated. Hence, the pressure change when the frame is exactly placed is detected.




Controlling clamping force

The clamping force can be changed to suit the workpiece by controlling the supplied air pressure.




Detecting tap breakage

Two opposed nozzles are supplied air at different pressures. If the tap breaks, the pressure at the lower pressure side nozzle is affected by the air of the higher pressure side nozzle. This change in pressure is detected.




Inspecting orientation of glass sheet

The orientation of the glass sheet can be recognized by detecting the change in vacuum due to presence / absence of indentation.



Controlling edge of winding film

With bifurcated nozzles placed on both sides of the film, the position of the winding film is recognized as right-shifted (high pressure), OK (middle pressure), or left-shifted (low pressure).



Analog voltage output incorporated as a standard

Since a linear analog voltage output (1 to 5 V) is incorporated, the sensor is ideally suited for real time monitoring or for remote control in combination with an analog controller (ultra-compact digital panel controller CA2 series, or digital panel controller CA series).


Peak hold / bottom hold display

The peak value or the bottom value of the varying pressure can be displayed. This function is convenient for finding the pressure variation range or for determining a reference for pressure settings.

Analog bar display


Pressure changes can also be displayed in an analog fashion using LED bars. Hence, sudden pressure changes can be recognized at a glance.


LED bars indicate the pressure level in steps of 10 % F.S., regardless of the pressure unit.




A Wide Variety of Models

Models are selectable according to mounting style, environmental resistance, and manner of use.







Flat type / DP2-4□

Direct mounting on a wall

The DP2 series covers worldwide usage with the Asian type, the North American type and the European type. Each type provides the customary pressure unit, suitable transistor output, and pressure port.

	Pres	sure unit			
	The interna- tional system of unit (SI)		Output	Pressure port	
Asian		kgf/cm² (Positive pressure type) mmHg (Vacuum pressure type)	NPN and	Rc (PT) ¹ / ₈ or M5 female thread	
North American	Pa	psi (Positive pressure type) inHg (Vacuum pressure type)		NPT ¹ / ₈ or NPTF ¹ / ₈ female thread	
European		bar	PNP and analog voltage	G (PF) ¹ / ₈ female thread	

ORDER GUIDE

DP2

	Ту	ре		Appearance	Rated pressure range	Model No.	Pressure port	Comparative output		
	Vacuum pressure	type	Asian			DP2-20	Rc (PT) ¹ / ₈ female thread	NPN open-collector		
	um pre	101 kPa type	rican		0 to - 101.3 kPa	DP2-20F	NPTF 1/8	transistor		
	Vacui		North American			DP2-20F-P	female thread	PNP open-collector transistor		
ırd	Standard	type	Asian	1000		DP2-21	Rc (PT) ¹ / ₈ female thread	NPN open-collector transistor		
standa		100 kPa type	North American	·0000	0 to 100.0 kPa	DP2-21F	NPTF ¹ / ₈	transistor		
o,	Positive pressure	10		0.00		DP2-21F-P	female thread	PNP open-collector transistor		
	ositive	ype	Asian	-		DP2-22	Rc (PT) ¹ / ₈ female thread	NPN open-collector transistor		
	_	MPa type	North American		0 to 1.000 MPa	DP2-22F	NPTF ¹ / ₈	transistor		
		_	Nort			DP2-22F-P	female thread	PNP open-collector transistor		
Light weight	Vacuum pressure	- 101 kPa type	Asian	-1000	0 to — 101.3 kPa	DP2-80	M5 female thread	NPN open-collector transistor		
	Λa	'	North American			DP2-40N	NPT ¹ / ₈ female thread			
at	Flat		European			DP2-40E	G (PF) ¹ / ₈ female thread	PNP open-collector transistor		
Ē		100 kPa type	Asian	CO. 100	0 to 100.0 kPa	DP2-41	Rc (PT) ¹ / ₈ female thread	NPN open-collector		
	ıre		North American	·(000 🏭		DP2-41N	NPT ¹ / ₈ female thread	transistor		
	Positive pressure	10	European	385		DP2-41E	G (PF) 1/8 female thread	PNP open-collector transistor		
	ositive	be/	_	Asian			DP2-42	Rc (PT) ¹ / ₈ female thread	NPN open-collector	
	ц	MPa type	North America		0 to 1.000 MPa	DP2-42N	NPT ¹ / ₈ female thread	transistor		
		_	Asian European			DP2-42E	G (PF) ¹ / ₈ female thread	PNP open-collector transistor		
	ssure	type				DP2-60	Rc (PT) ¹ / ₈ female thread	NPN open-collector		
	Vacuum pressure	III	O1 kPa North American	North American	THE PERSON NAMED IN	0 to - 101.3 kPa	DP2-60N	NPT ¹ / ₈ female thread	transistor	
	Vacu		European	-1000		DP2-60E	G (PF) ¹ / ₈ female thread	PNP open-collector transistor		
		100 kPa type	Asian		DP2-61	Rc (PT) 1/8 female thread	NPN open-collector			
IP67	re) kPa t) kPa t) kPa t	North American		0 to 100.0 kPa	DP2-61N	NPT ¹ / ₈ female thread
	pressu	10(European			DP2-61E	G (PF) ^{1/8} female thread	PNP open-collector transistor		
	Positive pressure	ed.	Asian	- 1		DP2-62	Rc (PT) ¹ / ₈ female thread	NPN open-collector		
	Ф	MPa type	North American		0 to 1.000 MPa	DP2-62N	NPT ¹ / ₈ female thread	transistor		
		=	European			DP2-62E	G (PF) ¹ / ₈ female thread	PNP open-collector transistor		

ORDER GUIDE


5 m 16.404 ft cable length type

5 m 16.404 ft cable length type is also available. (Standard: 2 m 6.562 ft)

		Туре		Standard	5 m 16.404 ft cable length type
				DP2-20	DP2-20-C5
	Vacuum pressure	- 101 kPa type	DP2-20F		
				DP2-20F-P	
	<u>p</u>			DP2-21	DP2-21-C5
•	Standard		100 kPa type	DP2-21F	
Ċ	ั้ง	Positive pressure		DP2-21F-P	
		Positive pressure		DP2-22	DP2-22-C5
			1 MPa type	DP2-22F	
				DP2-22F-P	
	ight			DP2-80	DP2-80-C5
	Light weight	Vacuum pressure	- 101 kPa type	DP2-40N	
	Ligh			DP2-40E	
				DP2-41	DP2-41-C5
Ċ	Flat	Positive pressure	100 kPa type	DP2-41N	
				DP2-41E	
				DP2-42	DP2-42-C5
			1 MPa type	DP2-42N	
				DP2-42E	
				DP2-60	
		Vacuum pressure	─ 101 kPa type	DP2-60N	
IP67			DP2-60E		
			DP2-61	The IDCZ towns in the attended	
		100 kPa type	DP2-61N	The IP67 type is the standard type with a 5 m 16.404 ft cable.	
	Positive pressure		DP2-61E		
	Source production		DP2-62		
		1 MPa type	DP2-62N		
				DP2-62E	

Accessories

- **DPX-01** [Pressure port attachment (Standard type only)]
- DPX-02 [Hexagon-socket-head plug for pressure port (Standard type only)]



OPTIONS

Designation	Model No.	Description					
Sensor mounting	MS-DPX	Mounting bracket for standard type [Two M4 (length 6 mm 0.236 in) pan head screws and two spring washers are attached.					
bracket (For standard type)	MS-DPX-4		ng bracket for standard type mm 0.236 in) pan head screws and two spring led.				
Straight bush	DPX-03	Changes the press male thread [R (PT)	sure port from female thread [Rc (PT) $^{1/8}$] to $^{1/8}$]				
Panel mounting bracket (For standard type)	MS-DPX-2	It can be used for mounting on a panel (1 to 3.2 mm 0.039 to 0.126 in thick).					
Front protection cover (For standard type)	DPX-04	It protects the sensor's adjustment panel. (It can be fitted when the panel mounting bracket is used.)					
Digital panel	CA2-T2	NPN open-collector transistor	This is a very small controller which allows two independent threshold level settings. • Supply voltage: 24 V DC ± 10 % • No. of inputs: 1 No. (sensor input) • Input range: 1 to 5 V DC • Main functions: Threshold level setting function, zero-adjust function, scale setting function, hysteresis setting function, autoreference function, power supply ON-delay function, etc.				
(Note)	CA-R2	Relay contact	This is a multi-functional controller having mathematical functions, hold function, etc. • Supply voltage: 100 to 240 V AC ± 10 % • No. of inputs: 2 Nos. (sensor inputs)				
	CA-T2	NPN open-collector transistor	Input range: 1 to 5 V DC Power supply for sensor: 12 V DC, 150 mA Main functions: Mathematical functions, process number				
	CA-B2	NPN open-collector transistor With BCD output	selection function, hold function, scaling function, auto-reference function, power supply ON-delay function, measurement start delay function, hysteresis setting function, etc.				


Note: For further details, refer to p.864 \sim for the ultra-compact digital panel controller **CA2** series, and to p.854 \sim for the digital panel controller **CA** series.

Sensor mounting bracket

· MS-DPX

• MS-DPX-4







Two M4 (length 6 mm 0.236 in) pan head screws and two spring washers are attached.


Straight bush

• DPX-03



Panel mounting bracket, Front protection cover

- MS-DPX-2 DPX-04



Digital panel controller

· CA2 series



· CA series



SPECIFICATIONS


			\/==					Danishua			
T				pressure					pressure		
//	Туре	01		Pa type	ID07		100kPa type	I	01	1MPa type	1
\ `			Light weight	Flat	IP67	Standard	Flat	IP67	Standard	Flat	IP67
\ \ \	Asian	DP2-20	DP2-80		DP2-60	DP2-21	DP2-41	DP2-61	DP2-22	DP2-42	DP2-62
Item\ \(\sigma\)	North American (Note)	DP2-20F(-P)		DP2-40N	DP2-60N	DP2-21F(-P)			DP2-22F(-P)		DP2-62N
				DP2-40E	DP2-60E		DP2-41E	DP2-61E		DP2-42E	DP2-62E
Type of p						Gauge p					
Rated pre	essure range			01.3 kPa) to 100.0 kP			to 1.000 MF	
Set press	sure range	$\left\{ \begin{array}{l} 0.052\ \text{to}\ -1.033\ \text{kgf/cm}^2, 0.051\ \text{to}\ -1.013\ \text{bar} \\ 0.74\ \text{to}\ -14.70\ \text{psi}, 38\ \text{to}\ -760\ \text{mmHg} \end{array} \right\} \qquad \left\{ \begin{array}{l} -0.051\ \text{to}\ 1.020\ \text{kgf/cm}^2 \\ -0.050\ \text{to}\ 1.000\ \text{bar} \end{array} \right\} \qquad \left\{ \begin{array}{l} -0.51\ \text{kgf/cm}^2 \\ -0.51\ \text{kgf/cm}^2 \end{array} \right\} $.050 to 1.000 .51 to 10.20 k .50 to 10.00 b .2 to 145.0 ps	gf/cm² ar	
Pressure	withstandability				490	kPa				1.47 MPa	
Applicable	e fluid					Non-corre	osive gas				
Selectabl	e units	kPa,	kgf/cm ² , bar	, psi, mmHg,	inHg	kPa	, kgf/cm ² , bar	r, psi	MPa	a, kgf/cm², ba	ır, psi
Supply vo	oltage				12 to 24 V	DC + 10 % F	Ripple P-P 10	% or less	•		
Current c	onsumption					50 mA					
(Compari Compari	tive outputs ative Output 1 ative Output 2	NPN open-c • Maximu • Applied vo	collector tran Im sink curre oltage: 30 V DC al voltage: 1		n comparative o	output and 0 V) current) current)	PNP open-o • Maximo • Applied v • Residu	collector tran um source ci voltage: 30 V D0	dard PNP out sistor urrent: 100 m C or less (betwee V or less (at	A en comparative	output and $+V$
Utiliz	ation category						or DC-13				
	out modes	Equipped v		mc	de (selectab	e, window cor le by key ope	ration)				ivity setting
Hyste	eresis			1 digit (howe		in hysteresis			using psi unit)	
Repe	eatability	Within ± 0.2 % F.S. ± 1 digit									
Resp	oonse time	2.5 ms or less									
Shor	t-circuit protection	Incorporated									
Analog voltage output		Output voltage: 1 to 5 V (over rated pressure range) Zero-point: within 1 V ± 5 % F.S. Span: within 4 V ± 5 % F.S. Linearity: within ± 1 % F.S. Output impedance: 1 kΩ approx. Approximately pressure (Positive pressure type)									
Display		31/2 digit red LED display (Sampling rate: 4 times/sec. approx.)									
	ayable pressure range	$ \left\{ \begin{array}{ll} 5.1 \text{ to} - 101.3 \text{ kPa} \\ 0.052 \text{ to} - 1.033 \text{ kgf/cm}^2, 0.051 \text{ to} - 1.013 \text{ bar} \\ 0.74 \text{ to} - 14.70 \text{ psi}, 38 \text{ to} - 760 \text{ mmHg} \\ 1.5 \text{ to} - 29.9 \text{ inHg} \end{array} \right\} \left\{ \begin{array}{ll} -5.0 \text{ to} 100.0 \text{ kPa} \\ -0.051 \text{ to} 10.20 \text{ kgf/cm}^2 \\ -0.050 \text{ to} 1.000 \text{ bar} \\ -0.72 \text{ to} 14.50 \text{ psi} \end{array} \right\} \left\{ \begin{array}{ll} -0.050 \text{ to} 1.000 \text{ MPa} \\ -0.51 \text{ to} 10.20 \text{ kgf/cm}^2 \\ -0.50 \text{ to} 10.00 \text{ bar} \\ -7.2 \text{ to} 145.0 \text{ psi} \end{array} \right\} $									
Analog ba	ar display	LED bar display in steps of 10 % F.S. approx.									
Operation		Orange LED (lights up when Comparative Output 1 is ON)									
indicators	Comparative Output 2			Gr	een LED (lig	hts up when (Comparative	Output 2 is 0	ON)		
	ition degree	3 (Industrial environment)									
Emcloumental resistance Ambinal Protest Insul Insul Vibra	ection	Standard, Flat and Light weight types: IP40 (IEC), IP67 type: IP67 (IEC)									
Amb	ient temperature	-10 to +50 °C +14 to +122 °F (No dew condensation or icing allowed), Storage: −10 to +60 °C +14 to +140 °F									
<u>∞</u> Amb	ient humidity	35 to 85 % RH, Storage: 35 to 85 % RH									
를 EWC	;	EN 50081-2, EN 50082-2, EN 61000-6-2									
₽ Volta	ge withstandability	1,000 V AC for one min. between all supply terminals connected together and enclosure									
<u>⊵</u> Insul	ation resistance	50 MΩ, or more, with 500 V DC megger between all supply terminals connected together and enclosure									
\ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \ \	ation resistance	10 to 150 Hz frequency, 0.75 mm 0.030 in amplitude in X, Y and Z directions for two hours each									
Shock resistance		100 m/s ² acceleration (10 G approx.) in X, Y and Z directions for three times each									
Temperature characteristics		Over ambient temperature range -10 to $+50$ °C $+14$ to $+122$ °F : within ± 1 % F.S. of detected pressure at $+20$ °C $+68$ °F									
	Asian		Standar	d, Flat and IF	P67 types: Ro	c (PT) ¹ / ₈ fema	ale thread, Li	ight weight ty	pe: M5 fema	le thread	
Pressure						nale thread, F			-		
port	European			71							
Material		Flat and IP67 types: G (PF) ¹ / ₈ female thread Front case: ABS, Rear case: PPS (glass fiber reinforced), Display surface: Acrylic Pressure port attachment: Die-cast zinc alloy [Light weight type: POM (glass fiber reinforced), pressure port is brass (nickel plated)] Front cover (IP67 type only): Polycarbonate									
Cable			0.15 m	m ² 5-core oil	resistant cab	tyre cable, 2	m 6.562 ft lo	ng (IP67 type	e: 5 m 16.404	ft long)	
Cable ext	tension	Extension up	to total 100 r	n 328.084 ft (le	ess than 10 m	32.808 ft wher	conforming to	o CE marking	is possible wi	th 0.3 mm ² , or	more, cable.
Weight		Star	dard type: 9	5 g approx.,	Flat type: 120	g approx., IF	P67 type: 370	g approx., I	_ight weight t	ype: 70 g app	orox.
Accessories		Hexagon-socket-head plug for pressure port: 1 pc. (Standard type only), Pressure unit label: 1 pc.									

Note: Model Nos. of North American standard type having the suffix '-P' are PNP output type.

I/O CIRCUIT AND WIRING DIAGRAMS

NPN output type

I/O circuit diagram

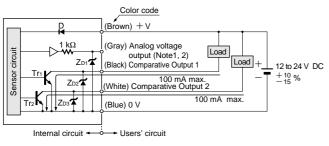


Notes:1) When using the analog voltage output, take care to connect external device of proper input impedance. Also, when a cable extension is used, voltage drop due to cable resistance should be taken into account.

2) The analog voltage output does not incorporate a shortcircuit protection circuit. Do not connect it directly to a power supply or a capacitive load.


Symbols ... D: Reverse supply polarity protection diode ZD1, ZD2, ZD3: Surge absorption zener diode Tr1, Tr2: NPN output transistor

Wiring diagram

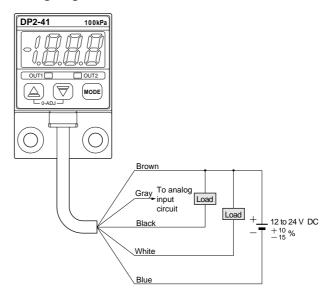

PNP output type

I/O circuit diagram

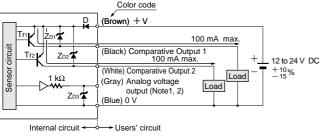


Notes:1) When using the analog voltage output, take care to connect external device of proper input impedance. Also, when a cable extension is used, voltage drop due to cable resistance should be taken into account.

2) The analog voltage output does not incorporate a shortcircuit protection circuit.

Do not connect it directly to a power supply or a capacitive load.

Symbols ... D: Reverse supply polarity protection diode Z_{D1}, Z_{D2}, Z_{D3} : Surge absorption zener diode T_{r1}, T_{r2} : PNP output transistor

Wiring diagram

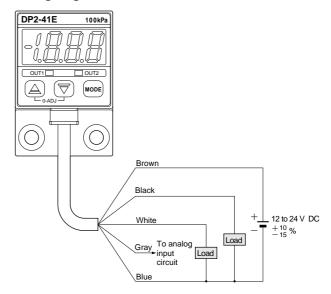

PRECAUTIONS FOR PROPER USE

All models




 This product is not a safety sensor. Its use is not intended or designed to protect life and prevent body injury or property damage from dangerous parts of machinery. It is a normal pressure detection sensor.

The DP2 series is designed for use with noncorrosive gas. It cannot be used with liquid or cor-

Operation

- If setting is impossible even with pressing the MODE key, verify whether the key-protect function is enabled. Please note that pressing down on the MODE key for an extended moment will enable the key-protect function as soon as the key is released.
- If using the window comparator mode, set the pressure value so that there is a difference of 3 digits, or more, between Set Value 1 (P-1) and Set Value 2 (P-2). No output will be possible with a 0 to 2 digit difference.

Functional description



	Description	Function					
1	31/2 digit LED display (Red)						
2	Comparative Output 1 operation indicator (Orange) Lights up when Comparative Output 1 is ON						
3	Comparative Output 2 operation indicator (Green)	Lights up when Comparative Output 2 is	ON.				
4	Increment key (()	In the initial setting mode, pressing the key changes the settable digit. In the Set Value 1, 2 modes, pressing the key changes the set value to the high pressure side in case of positive pressure type sensor and to the high vacuum side in case of vacuum pressure type sensor. In the sensing mode, if the key is pressed continuously for 4 sec. or more, the display shows peak hold value.	oth the keys are pressed nt adjustment is done.				
(5)	Decrement key ((▽)	In the initial setting mode, pressing the key changes the set conditions. In the Set Value 1, 2 modes, pressing the key changes the set value to the low pressure side in case of positive pressure type sensor and to the low vacuum side in case of vacuum pressure type sensor. In the sensing mode, if the key is pressed continuously for 4 sec. or more, the display shows bottom hold value.	In the sensing mode, if both the keys are pressed simultaneously, zero-point adjustment is done.				
6	Mode selection key	Each press of the key changes the sele mode to sensing mode, Set Value 1 (P-1 mode and Set Value 2 (P-2) set mode. In the sensing mode, if the key is precontinuously for about 3 sec., key-protect be set / released. In the sensing mode, if the mode selekey is pressed while pressing the increakey (), the initial setting mode is obtain	ssed t can ction ment				

Error messages

• When an error occurs, take the following corrective action.

Error message		Cause	Corrective action		
<u>E-1</u>	Overcur circuit.	rrent due to short-	Switch off the power supply and check the load.		
<u> </u>		e is being applied zero-point adjust-	Applied pressure at the pressure port should be brought to atmospheric pressure and zero-point adjustment should be done again.		
	Positive pressure type	Applied pressure exceeds the upper limit of displayable pressure range.			
	Vacuum pressure type	Applied pressure exceeds the lower limit of displayable pressure range.	Applied pressure should be		
	Positive pressure type	Applied pressure exceeds the lower limit of displayable pressure range.	brought within the rated pressure range.		
	Vacuum pressure type	Applied pressure exceeds the upper limit of displayable pressure range.			

Wiring

The analog voltage output does not incorporate a shortcircuit protection circuit. Do not directly connect a power supply or a capacitive load.

- Make sure that the power supply is off while wiring.
- Verify that the supply voltage variation is within the rating.
- If power is supplied from a commercial switching regulator, ensure that the frame ground (F.G.) terminal of the power supply is connected to an actual ground.
- In case noise generating equipment (switching regulator, inverter motor, etc.) is used in the vicinity of this sensor, connect the frame ground (F.G.) terminal of the equipment to an actual ground.
- Do not run the wires together with high-voltage lines or power lines or put them in the same raceway. This can cause malfunction due to induction.

Conditions in use for CE conformity

• The **DP2** series is a CE conformity product complying with EMC Directive. The harmonized standard with regard to immunity that applies to this product is EN 61000-6-2 (Note) and the following condition must be met to conform to that standard.

• The sensor should be connected less than 10 m 32.808 ft from the power supply.

Note: The EN 50082-2 that previously applied to the products for conforming to EMC Directive was replaced by EN 61000-6-2 starting April 1st, 2002.

PRECAUTIONS FOR PROPER USE

All models

Setting

- If key-protect has been set, make sure to release key-protect before operating the keys. (Please refer to 'Key-protect function' on p.801 for the procedure.)
- Set Value 1 (P-1) and Set Value 2 (P-2) can be made common for all the output modes.
- The setting of Set Value 2 (P-2) with respect to Set Value 1 (P-1) can only be towards the high pressure side in case of the positive pressure type sensor and only towards the high vacuum side in case of the vacuum pressure type sensor.
- Set Value 3 (P-3) is automatically set to the mid-value of Set Value 1 (P-1) and Set Value 2 (P-2). (When setting the pressure value for the automatic sensitivity mode)
- The conditions which are set are stored in an EEPROM. Kindly note that the EEPROM has a life span and its guaranteed life is 100,000 write operation cycles.

Setting procedure

1 Zero-point adjustment

Adjust zero-point

2 Initial setting

Set 'Display', 'Output mode', and 'Unit'

1 Zero-point adjustment

 The displayed pressure when the pressure port is left open is adjusted to zero.




- The sensor will automatically enter the sensing mode when power is supplied.
- · Let the pressure port be at atmospheric pressure (i.e., no applied pressure condition), and press, simultaneously, the increment and decrement keys continuously.
- \[\text{\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\}\$}}}}}}}}} \end{linethinteristinf{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\exitil{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\text{\$\ released, zero-point adjustment is completed and the sensor returns to the sensing mode.

2 Initial setting

· Pressure 'Unit', 'Display' and 'Output mode' of the comparative outputs are set.



- In the sensing mode, press we key while pressing (a) key.
- . Initial setting is displayed.
- If sensor is being used for the first time, PHD is displayed.
- The settable digit blinks.
- The settable digit changes when 👜 key is



3 Pressure value setting

Enter Set Value 1 (P-1), Set Value 2 (P-2), Set Value 3 (P-3)

Measurement

Commence measurement on completion of setting

③ Pressure value setting

For the case when output mode is set to either hysteresis mode (H), window comparator mode (L) or dual output mode (♂).

· 'Set Value 1 (P-1)' and Set Value 2 (P-2)' of the comparative outputs are set.



- Press week key in the sensing mode to set to Set Value 1 (P-1) set mode.
- Enter Set Value 1 (P-1) using

 key and

 key.
- Then, press week key to set to Set Value 2 (P-2) set mode.
- Then, press week key to set to sensing mode.

For the case when output mode is set to automatic sensitivity setting mode ($\ensuremath{\mathcal{R}}$).

'Set Value 1 (P-1)', 'Set Value 2 (P-2)' and 'Set Value 3 (P-3)' of the comparative outputs are set.



Value 1 (P-1) set mode. · Within the required permissible pressure range, having created a pressure state which is nearest

• Press woe key in the sensing mode to set to Set

- enter Set Value 1 (P-1).
- Then, press week key to set to Set Value 2 (P-2) set mode.
- · Within the required permissible pressure range, having created a pressure state which is nearest to the high pressure end (for a positive pressure type sensor) or the high vacuum end (for a vacuum pressure type sensor), press (key to enter Set Value 2 (P-2).
- Then, press key to set to Set Value 3 (P-3)
- · Check Set Value 3 (P-3) which has been set automatically. When Set Value 3 (P-3) is to be changed, enter Set Value 3 (P-3) using (a) key
- After checking and setting, press key to set to sensing mode.
- The automatically set Set Value 3 (P-3) can be manually changed to a value between Set Value 1 (P-1) and Set Value 2 (P-2).
- · If using the window comparator mode, set the pressure value so that there is a difference of 3 digits, or more, between Set Value 1 (P-1) and Set Value 2 (P-2). No output will be possible with a 0 to 2 digit difference.

PRECAUTIONS FOR PROPER USE

All models

Conversion of pressure units

• In the DP2 series, the conversion to different units is automatically done on changing the setting of the pressure unit. However, this conversion can also be obtained by multiplying the values by the coefficients given in the table on the right.

Conversion procedure

· For example, if 2 kPa is to be expressed in kgf/cm2,

since 1 kPa = 1.01972×10^{-2} kgf/cm², 2 kPa becomes

 $2 \times 1.01972 \times 10^{-2} = 0.020 \text{ kgf/cm}^2$.

Conversion table for pressure units

	kPa	MPa	kgf/cm ²	bar	psi	mmHg (Torr)	inHg	atm
1 kPa	1	1×10 ⁻³	1.01972×10 ⁻²	1×10 ⁻²	1.45038 × 10 ⁻¹	7.50062	0.2953	9.86923×10 ⁻³
1 MPa	1×10³	1	1.01972×10	1×10	1.45038 × 10 ²	7.50062×10^{3}	0.2953×10^{3}	9.86923
1 kgf/cm ²	9.80665×10	9.80665×10 ⁻²	1	9.80665×10 ⁻¹	1.42234×10	7.35559 × 10 ²	2.8959 × 10	9.67841 × 10 ⁻¹
1 bar	1×10²	1×10 ⁻¹	1.01972	1	1.45038×10	7.50062 × 10 ²	2.953×10	9.86923×10 ⁻¹
1 psi	6.89473	6.89473×10 ⁻³	7.03065×10 ⁻²	6.89473×10 ⁻²	1	5.17147×10	2.036	6.80457×10 ⁻²
1 mmHg (1 Torr)	1.33322 × 10 ⁻¹	1.33322×10 ⁻⁴	1.35951 × 10 ⁻³	1.33322×10 ⁻³	1.93368×10 ⁻²	1	3.9370×10 ⁻²	1.31579×10 ⁻³
1 inHg	3.3864	3.3864×10 ⁻³	3.4531 × 10 ⁻²	3.3864×10 ⁻²	0.4912	2.5400×10	1	3.342 × 10 ⁻²
1 atm	1.01325 × 10 ²	1.01325 × 10 ⁻¹	1.03323	1.01325	1.46960×10	7.60000 × 10 ²	2.9921 × 10	1

Key-protect function

· Key-protect is a function which prevents any unintentional change in the conditions which have been entered in each setting mode by making the sensor not to respond to the key operations.

Setting of key-protect



- In the sensing mode, press week key continuously for about 3 sec. and release it immediately when
- (Key-protect is set and the sensor returns to the sensing mode.

Release of key-protect



- \bullet In the sensing mode, press $\ensuremath{\mbox{\tiny{MODE}}}$ key continuously for about 3 sec. and release it immediately when \[
 \textit{UFF} \]
 is displayed.
 \]
 - · Key-protect is released and the sensor returns to the sensing mode.

Others

- Use within the rated pressure range.
- · Do not apply pressure exceeding the pressure withstandability value. The diaphragm will get damaged and correct operation shall not be maintained.
- Do not use during the initial transient time (0.5 sec.) after the power supply is switched on.
- Avoid use of standard type, flat type and light weight type of sensors in places where steam and dust is excessive.
- Take care that the sensor does not come in direct contact with water, oil, grease, or organic solvents, such as, thinner, etc.
- Do not insert wires, etc., into the pressure port. The diaphragm will get damaged and correct operation shall not be maintained.
- Do not operate the keys with pointed or sharp objects.


PRECAUTIONS FOR PROPER USE

Standard type

Setting of pressure lead direction

•The pressure lead direction can be changed by dismantling the pressure port attachment and changing the mounting direction. The tightening torque of the hexagon-socket-head bolt (length: 9 mm 0.354 in or less) should be 0.29 N·m or less.


Note: Make sure to close any unused pressure port with the hexagonsocket-head plug supplied as accessory.



Piping


· When connecting a hexagon-socket-head plug or coupling to the pressure port, hold the hexagonal part of the pressure port with a 12 mm 0.472 in spanner and make sure that the tightening torque is 9.8 N·m or less. Also, in order to prevent any leakage, wind a sealing tape on the coupling when connecting.

However, sealing tape is not required for North American type (DP2-DFD) using NPTF 1/8 coupling. (Sealing tape is required if NPT 1/8 coupling is used.)



Mounting


• When mounting the sensor with the sensor mounting bracket, etc., the tightening torque should be 1.2 N·m or



Flat type Light weight type


Setting of pressure lead direction

•The pressure lead direction can be changed by dismantling the pressure port attachment and changing the mounting direction. The tightening torque of the hexagon-socket-head bolt (length: 9 mm 0.354 in or less) should be 0.29 N·m or less.

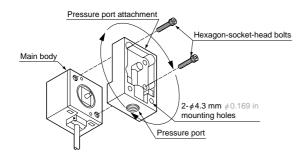

Piping

• When connecting a coupling to the pressure port, hold the pressure port attachment with a 16 mm 0.630 in (light weight type: 10 mm 0.394 in) spanner and make sure that the tightening torque is 9.8 N·m or less (light weight type: 1.47 N·m or less). Also, in order to prevent any leakage, wind a sealing tape on the coupling when connecting.



PRECAUTIONS FOR PROPER USE


IP67 type

Piping for pressure measurement inlet port

• When connecting a coupling to the pressure measurement inlet port, hold the pressure port attachment with a spanner and make sure that the tightening torque is 9.8 N·m or less. Also, in order to prevent any leakage, wind a sealing tape on the coupling when connecting.


Piping for atmospheric pressure inlet port

· If there is a possibility of water entering into the sensor enclosure through the atmospheric pressure inlet port, connect a tube to the atmospheric pressure inlet port through a M5 coupling and extend the other end of the tube to a safe place. In this case, ensure that this end of the tube does not get clogged.




Fitting of front cover


• Insert the bosses on the front cover into the guide holes at the bottom of the pressure port attachment, and push in the direction of the arrow to fit the hook. When removing the front cover, release the hook first.




DIMENSIONS (Unit: mm in) The CAD data in the dimensions can be downloaded from the SUNX website: http://www.sunx.co.jp/

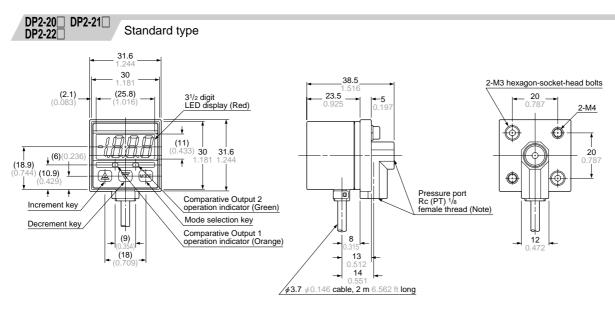


Note: NPTF 1/8 female thread for North American type.

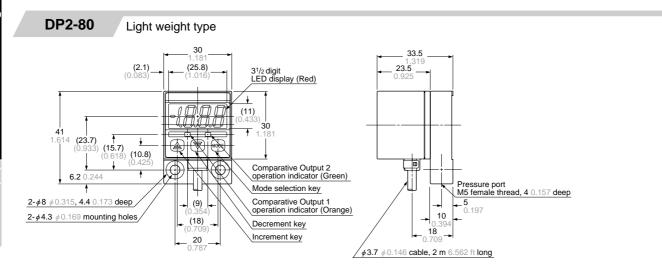

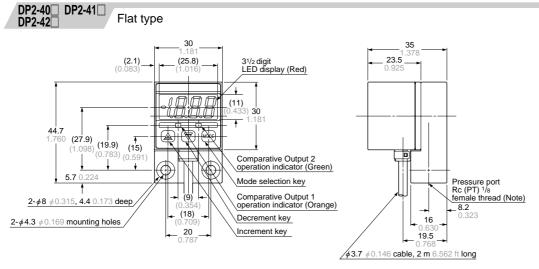

Note: NPT 1/8 female thread for North American type, and G (PF) 1/8 female thread for European type.


DIMENSIONS (Unit: mm in) The CAD data in the dimensions can be downloaded from the SUNX website: http://www.sunx.co.jp/

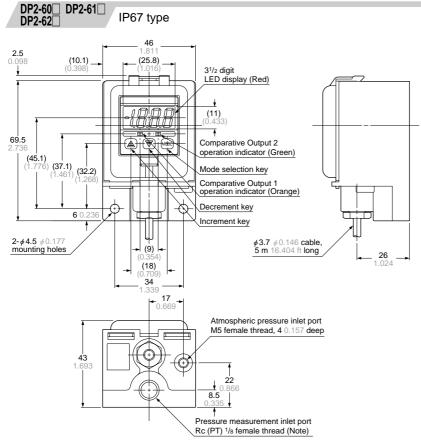


Note: NPT 1/8 for North American type, and G (PF) 1/8 for European type.

MS-DPX

Sensor mounting bracket for standard type (Optional)

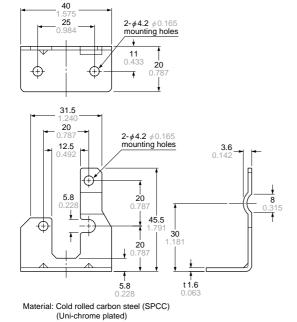


Assembly dimensions

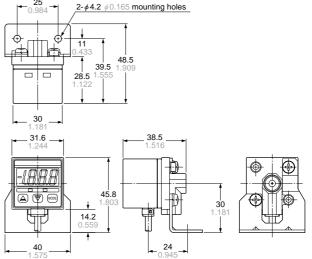


DIMENSIONS (Unit: mm in) The CAD data in the dimensions can be downloaded from the SUNX website: http://www.sunx.co.jp/

MS-DPX-4

Back angled mounting bracket for standard type (Optional)



Assembly dimensions

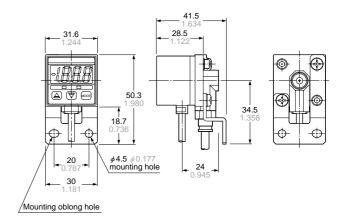


Material: Cold rolled carbon steel (SPCC) (Uni-chrome plated)

Two M4 (length 6 mm $0.236\ \text{in}$) pan head screws and two spring washers are attached.

MS-DPX-2 DPX-04

Panel mounting bracket, front protection cover for standard type (Optional)

Assembly dimensions

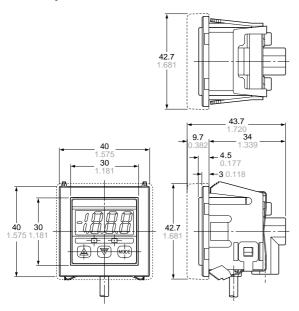


portion shows the front protection cover.

Material: Polycarbonate (Front protection cover)

Nylon 6, Stainless steel (SUS304)(Panel mounting bracket)

Panel cut-out dimensions



Note: The panel thickness should be 1 to 3.2 mm 0.039 to 0126 in.